

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 20 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130308</u>	
Name <u>Michael A. Wery</u>		ID# <u>3590</u>	Date <u>4-23-10</u>
A	Agency <u>AST</u>	Phone # <u>451-2550</u>	
Instrument Location <u>Healy Post</u>			
Alco S/N <u>X173355</u>		Target Value <u>.082</u>	High Pressure <u>100 psi</u>
B	Alco Test Value Average <u>.077</u>		
	1 st Alco	2 nd Alco	
Signature <u>[Signature]</u>		<u>COB</u> <u>5/24/10</u>	
(OVER)			

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of June, 2010.

[Signature]
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

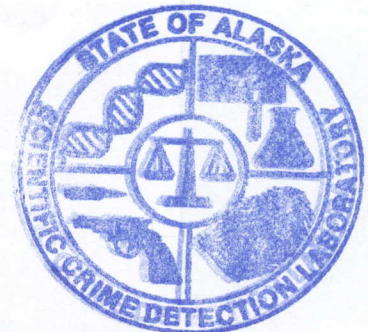

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130308 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130308 ✓

APRIL 23, 2010 ✓ *cos Sp24/10*

OPERATOR'S NAME:
WERY/MICHAEL/A
OPERATOR'S NUMBER: 3590
SUBJECT'S LAST NAME:
VERIFICATION
SUBJECT'S FIRST NAME/MI :
OF CALIBRATION
O.L. #: 0
DEPT/AGENCY: HLY0
CASE/REPORT:
TEST TYPE: V
ALCO TARGET VALUE: .002 ✓
ALCO S/N: X173355 ✓

— BREATH ANALYSIS —

.002 ADJUSTED FOR 28.68 in
ALCO TARGET .078 11:40
BLANK TEST .000 11:41
INTERNAL STANDARD VERIFIED 11:41
ALCO TV 28.68 in .077 11:41
BLANK TEST .000 ✓ 11:42
SUBJECT SAMPLE *cos Sp24/10* .000 11:42
BLANK TEST .000 11:43
ALCO TV 28.68 in .077 11:44
BLANK TEST .000 ✓ 11:44

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130308 ✓

APRIL 23, 2010 ✓
TIME 11:37

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 42c
BAROMETER: 28.68 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

'###'()*+,-./0123456789:;<=>?@AB CDEFG
HIJ KLMNOPQRSTU VWXYZ[\]^_`abcde fghijklmno
pqrstuvwxy z{ }~|